

HOW TO PERFORM RAPID TEST FOR MALARIA

Training for the use of First Response® Malaria Ag. P.f. (HRP2) / P.f. (pLDH) / P.v. (pLDH) Test Detects Malaria Ag. *P.falciparum* specific to pLDH and HRP2 and *P.vivax* specific to pLDH in human whole blood

- New unopened test device pouch
- New unopened alcohol swab
- New unopened lancet
- New pair of disposable gloves
- Assay Buffer Bottle
- Timer
- Biohazard waste container
- Non-biohazard waste container
- Permanent Marker



Disposable gloves



Alcohol swab



Permanent Marker



Specimen Transfer Device



Lancet



Timer




Assay Buffer Bottle



Test device pouch

READ THE INSTRUCTIONS CAREFULLY BEFORE PERFORMING THE TEST.


1. Check expiry date on the test pouch.
(If expired, do not use)

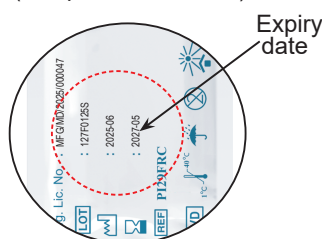

2. Put on gloves. Use new gloves for each patient.



3. Open the pouch and remove:



a. Test Device


b. Desiccant

Desiccant Validity
Orange: Valid
Green: (Do not use the test device if the desiccant turns green).


4. Label the test device with patient identification number/name



5. Wipe the patient finger with alcohol swab.
(Alcohol must be dry before pricking)



6. Take the lancet and detach the cap of the lancet and pierce the finger with the lancet.

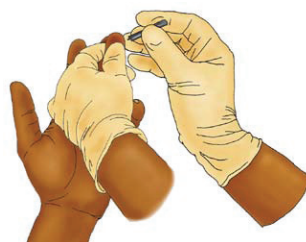


7. Dispose the lancet immediately into the sharps box.



8. Take the specimen transfer device and collect 5 µl of blood by touching the circular end of the specimen transfer device into the blood drop.




9. Touch the specimen transfer device into the specimen well vertically.

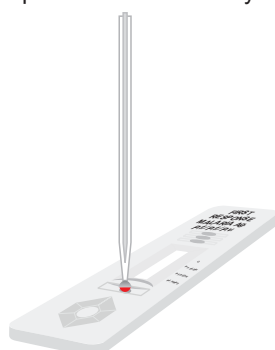

10. Dispose the used specimen transfer device into the biohazardous container.



11. Add two drops of assay buffer into the buffer well vertically.




12. Interpret the result at 20 minutes.



13. Do not Interpret after 30 minutes.

14. How to interpret test results.

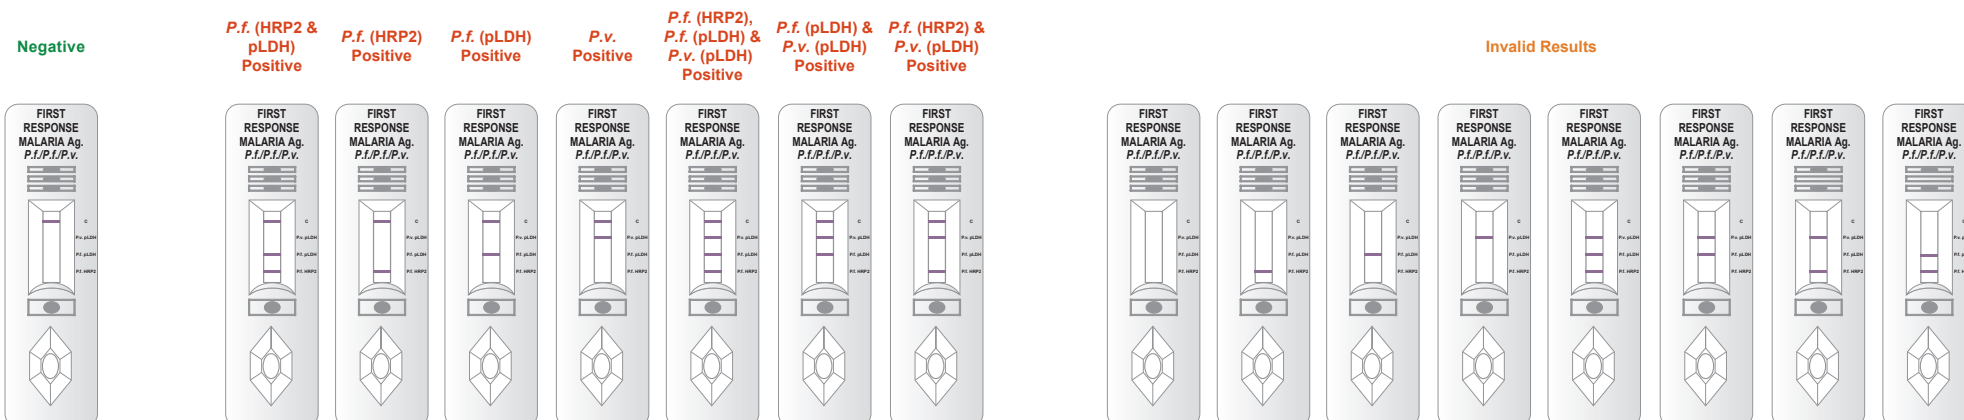

The invalid test results should be retested with new test device.

15. Record the test results. Dispose of used test device into biohazard waste container.



16. Dispose off desiccant and used gloves in a biohazardous waste container. Dispose off the packaging materials in a non-biohazard waste container.



NOTE: Do not re-use the test device, alcohol swab, lancet and specimen transfer device as are intended for single use only

Manufactured by



Premier Medical Corporation Private Limited

A1-302 and 3704-05, GIDC Sarigam, Valsad, Gujarat (India) - 396155
• Customer support email : info@premiermedcorp.com • Tel.: +91 260 2780112/113,
• www.premiermedcorp.com
An ISO 13485 & EN ISO 13485 Certified Company