

JOB AID

For more detailed instructions please refer to Instructions for use.

FIRST RESPONSE[®] HCV Card Test (Self Test) (Whole Blood)



Training in the use of First Response[®] HCV Card Test (Self Test) that is intended to use for self-testing by untrained/lay user as an aid to detect antibodies specific to HCV in human whole blood.

Please read instructions for use completely, prior to use.

All components must be brought to room temperature (between 15-30°C) prior to testing.

Caution:
DO NOT USE THE TEST DEVICE AND ANY COMPONENTS MORE THAN ONCE.

Materials Provided

• Each self test pack contents:
Test device with desiccant & Specimen transfer device,
Alcohol swab, Dry swab, Bandage, Sterile lancet,
Assay buffer vial, Instructions for use, Biohazard bag.

Materials required but not provided:
Clock, watch or timing device

HOW TO USE THE FIRST RESPONSE[®] HCV CARD TEST (SELF TEST)



Before starting the test procedure, wash your hands, preferably with warm water and soap, and dry them completely before testing. Check the expiry date of the test device.

Open the test device pouch by tearing along the notch and verify the pouch contents.


Wipe your fingertip by using the alcohol swab and allow it to dry for approximately 15 seconds.

Carefully remove the clear protective cap of the sterile safety lancet provided.

Place the uncapped lancet over the cleaned fingertip and press down firmly to prick your skin with the needle.

Gently squeeze your fingertip to obtain a large first drop of blood.

Wipe the first drop of the blood away using dry swab provided.

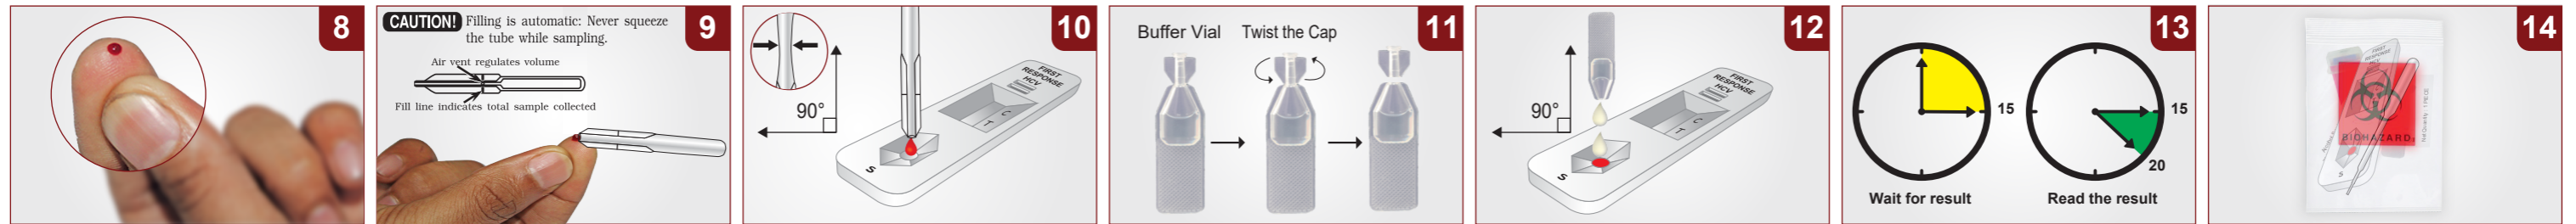

Without pressing too hard, gently squeeze your fingertip once again to obtain a large second drop of blood.

Hold the tube horizontally, and touch the tip of specimen transfer device to the blood. Capillary action will automatically draw the blood to the fill line (35µl) and stop.

Place the test device on a flat, clean and dry surface. Align the tip of the tube with sample well and squeeze the bulb.
Note: If sample won't expel, you probably didn't allow the tube to fill all the way. Touch the tip to the blood sample again and allow it to fill completely. Then align the tip with the sample well and squeeze the bulb.

Take the assay buffer vial provided and twist the cap to open single use assay buffer vial as shown in the above figure.

Gently press the single use assay buffer vial to add 2 drops of assay buffer to the specimen well (S). Wait for 15 minutes. Meanwhile, apply bandage to the finger.

Read the test result at 15 minutes. Do not interpret after 20 minutes.


After reading test result dispose of all used kit contents as infectious waste, into the biohazardous bag provided.

RESULT, INTERPRETATION AND FOLLOW UP



Read test result in a well-lit area


Non-reactive (Negative) result



If only one color line appears at control line 'C' as in the figure, the specimen is non-reactive (negative).


Follow Up: Seek regular testing. If you may have been exposed to HCV, repeat the test again in 3 months.

Reactive (Positive) result




If two color lines appear, one at control line 'C' and the other at test line 'T' as in the figure you may be HCV positive and should seek additional testing and medical care.

Follow Up: As soon as possible, visit your nearest HCV Testing Center or Health Facility.



Presence of faint line at test line 'T' as shown in figure you may be HCV positive and should seek additional testing and medical care.

Invalid result

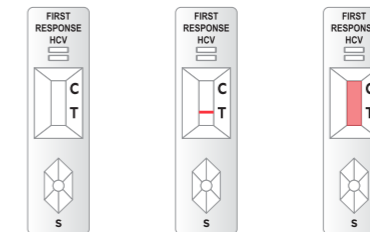

No presence of control line 'C' in the result window (irrespective of presence of test lines) or a red background makes it impossible to read the test results indicates an invalid result. The directions may not have been followed correctly and should be retested with new test device.

Follow Up: If the test did not work properly. You must repeat the test or visit your nearest HCV testing center or health facility.



Manufactured by
Premier Medical Corporation Private Limited
A1-302, GIDC, Sarigam-396155, Dist. Valsad, Gujarat, INDIA.
Customer support email: info@premiermedcorp.com
Tel: +91 260 2780112/113, www.premiermedcorp.com



ISO 13485 & EN ISO 13485
Certified Company